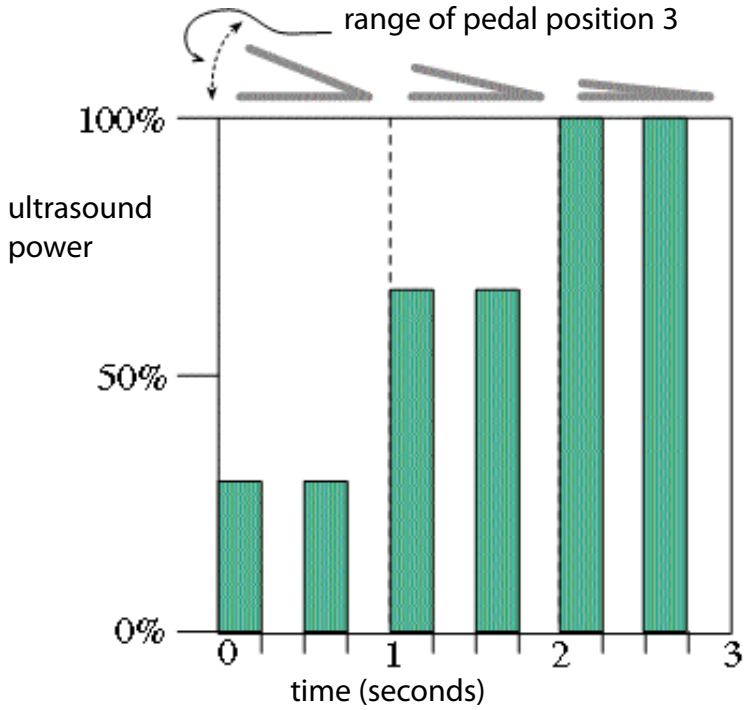

Pulse Mode
Linear ultrasound power
machine panel settings:
power:
minimum: 0%
maximum: 100%
Pulses per second (pps):
2 pps
Foot pedal is sequentially depressed to three positions within position 3:
1st second: 1/3 depressed
2nd second: 2/3 depressed
3rd second: fully depressed

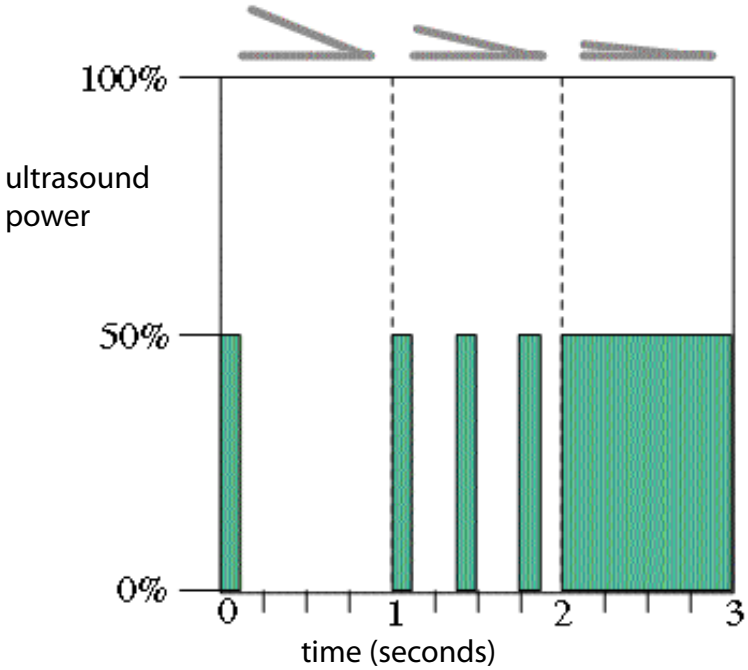

Burst Mode
Fixed ultrasound power
machine panel settings:
power:
50%

Burst duration: 125 msec

Foot pedal is sequentially depressed to three positions within position 3:
1st second: 1/3 depressed
2nd second: 2/3 depressed
3rd second: fully depressed

FIGURE 1-55